

Positioning and Smoothing Movement Approaches of a Linear Actuator Dedicated to A Biomedical Application

Imed Mahmoud¹ and Adel KHEDHER¹

¹ Laboratory of Advanced Technology and Intelligent Systems (LATIS)

¹Mahmoud.Imed@issatm.rnu.tn, adel_kheder@yahoo.fr

Abstract: The movement of linear stepper motors is characterized by a highly oscillatory translation, which is troublesome for the positional accuracy and the speed constant (often required by many industrial applications such as the syringe pump). These oscillations can lead to loss of synchronism and stall risk. Thus, in order to attenuate the amplitudes of these oscillations and to guarantee the positioning of the actuator without errors, solutions exploiting open-loop and closed-loop control techniques are proposed in this paper for the purpose of improve the performance of the actuator.

Keywords: Linear Actuator, Syringe Pump, Oscillations, Dynamic Response, Bang-Bang, Closed Loop Control and Precision.

1. Introduction

The syringe pump is a conventional biomedical system hospital emergency service. It is mainly used for intravenous, intra-arterial infusions, anesthetic infusions and chemotherapy. It is essential in the various departments of general surgery and the internal department of medicine for children, adults, pediatrics, the emergency department, gynecology, etc.

In the case of diseases affecting the patient's therapeutic area, such as renal insufficiency, the frequent administration of drugs leads according to the dose administered to two possible cases, [1]:

- If the dose is low, the drug becomes useless although there is a residual concentration maintained in the body. Thus, the mean value of the drug concentration is included in the ineffective zone, Figure.1.
- When the dose is too high, the average evolution of the concentration is carried in the toxic zone; the undesirable effects then become very important compared to the efficiency.

The pharmacokinetics of these two oral administration cases is illustrated in Figure.1.

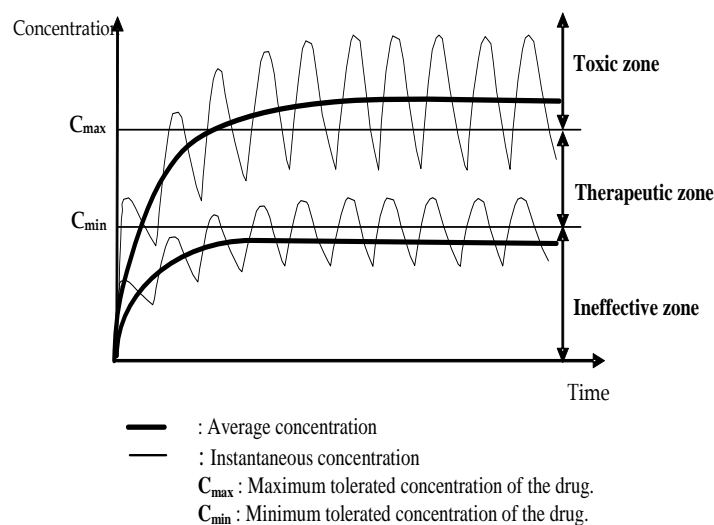


Fig.1- Pharmacokinetics of oral administration.

For such cases of diseases where the therapeutic zone is reduced, the maintenance of a concentration evolving without exceeding in this zone cannot be guaranteed by use of an oral administration. The use of an infusion is then a necessity.

Perfusion is a drug delivery method continuously over a constant rate. The plasma concentration increases until, for the same unit of time, the dissipated amount equates which is administered by infusion. This results in a plateau whose height at steady state depends on the rate of infusion and the concentration of the drug in the administered solution, Figure 2. Maintaining this equilibrium state is conditioned by the nature of the infusion solution, the infusion rate and duration of care. Moreover, they are in dependence on the patient's condition, age and weight, [2].

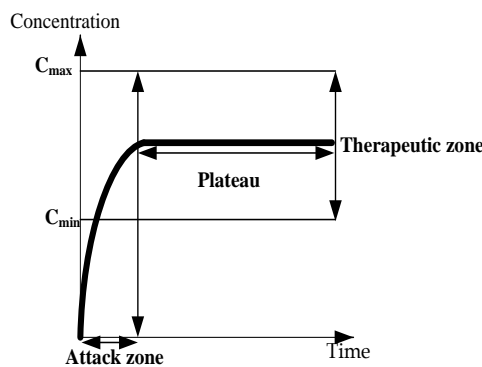


Fig.2- Pharmacokinetics of an infusion.

In the case of diseases with renal or cardiovascular insufficiency, the patient is subjected to treatment requiring infusions at high concentrations over a long period, with adjustable speed and precise rhythm, [1]. Therefore, it was necessary to set up the programmable automatic syringe (time, flow, period) whose technology is constantly evolving for the search for performance improvement. The block diagram of the all biomedical system (syringe pump), to be modelled, is illustrated by Figure 3 where all geometrical parameters are defined.

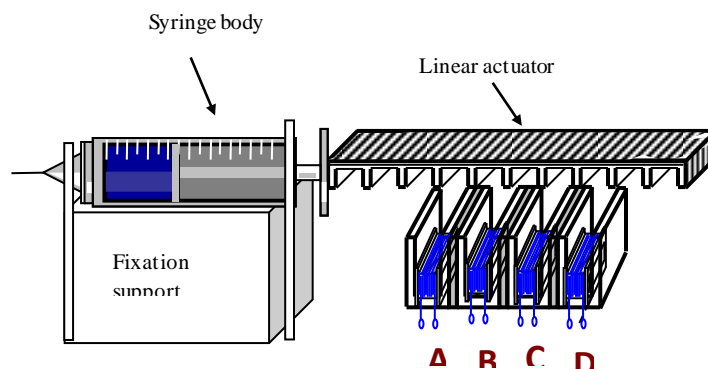


Fig.3- The proposed motorization solution.

Some significant characteristics of the actuator and syringe are given in table 1 and 2.

Table 1. Motor mechanical and electrical parameters

Number of modules	4
Tooth width	3mm
Slot width	3mm
Tooth pitch	6mm
Phase separation	1.5mm
Mover length	135 mm
stator length	40.5 mm
Air gap width	0.1mm
Height of the stator teeth	17mm
Height of the mover teeth	4mm
Depth of the actuator	30mm
Number of turns per phase	520

Table 2. Dimensions of the used syringe.

volume of the syringe	60 ml
Piston mass	15 g
Length of the cylinder	118 mm
External diameter of the cylinder	30.11 mm
Internal diameter of the cylinder	27.48 mm
Tube length	1600 mm
Inner diameter of the tube	3.7 mm
Needle length	69.7 mm
Needle diameter	0.8 mm
Required thrust force	4N
rated voltage	14 V
rated current	1 A

The movement of a stepper motor presents oscillations often generating vibrations and acoustic noise and can even, at certain operating frequencies, induce synchronism losses and chaotic operation cases. This unwanted operation is manifested by a start in jerky motion causing danger, a loss of synchronism leading to an eminent stall. These oscillations influence the evolution of the drug in the body. Therefore, the effectiveness of the drug that is on the patient's health.

Conventionally, when incremental displacement without vibrations or oscillations is required, two technological concepts are generally used for movement smoothing. The first involves improving the mechanical manufacture of the motor itself. The contributions in this case are often difficult, cumbersome and expensive. The second concept uses damping techniques ensured by the adaptation of laws and adequate control systems. Moreover, the research results obtained have shown that the characteristics of the thrust force developed by the linear actuator cannot be assimilated to sinusoids and that they are strongly influenced by the magnetic state and the geometries of the actuator.

The approach in this paper is to suggest control approaches taking into account the dynamic behavior ensuring precise positioning and without overshoot for different medication infusion rates.

2. Open loop control method (Bang Bang)

The oscillation damping of a stepping motor can be ensured by the successive excitation of two adjacent stator phases. Indeed, by exciting phase B until time t_1 , the rotor is brought to a position close to its natural equilibrium, figure.4. At this time, a power supply switch is turned on to energize phase A and de-energize phase B. This power configuration where the coil of phase B is de-energized and the coil of phase A is energized remains locked until at time t_2 . If the interval $[t_1-t_2]$ is well adjusted, the amount of energy produced by phase A compensates exactly the kinetic energy accumulated during the movement. Then, to keep the rotor in the targeted position, the supply of phase B is restored at time t_2 . Thus, the braking force imposed by the excitation of phase A attenuates the oscillations and allows the rotor to reach its equilibrium position without overtaking.


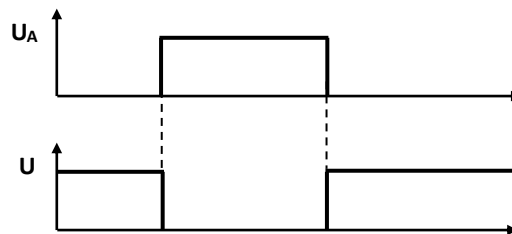



Fig.4-Applied voltage.

The determination of switching times t_1 and t_2 are strongly related to the stepper motor controlled, [4-5-6-7-8-9].


In the event of operation, phase B is considered as the driving phase and phase A is used for braking. The application by Bang-Bang control simulation, for switching times $t_1 = 50$ ms and $t_2 = 80$ ms and for a voltage of 18 V, allows the attenuation of the overruns observed at the position evolution. The determination of the appropriate switching times t_1 and t_2 has been adjusted several simulation tests. Figure.5 shows the evolution of the currents in the driving phase and in the braking phase. Consequently, the current generated in phase A allowed the motor braking and the damping observed on the position evolution.

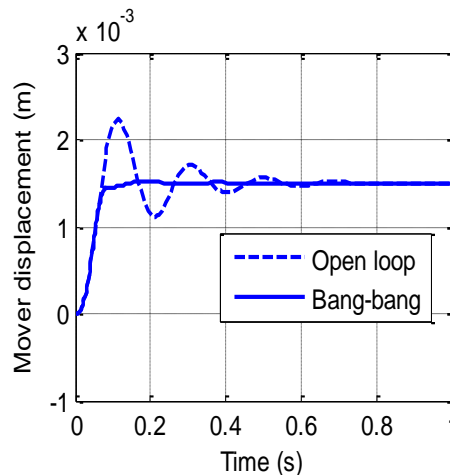


a)

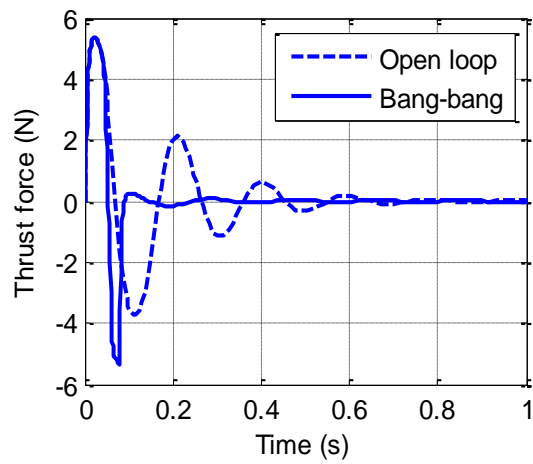

b)

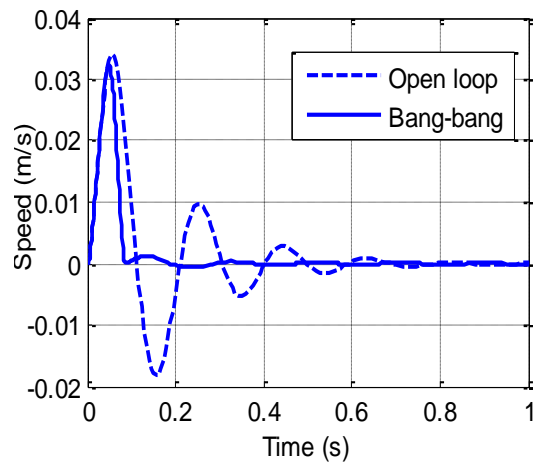

c)

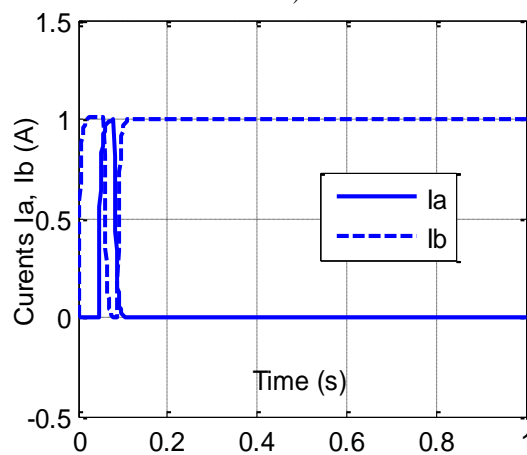

d)

Fig.5- Amortization of rotor oscillations by application of the "Bang-Bang" method.

(a) : Mover displacement (b) : Thrust force (c) : Speed (d) : Control current.

Comparing these results to those corresponding to full-step operation; it is remarkable that the "Bang-Bang" command provides indisputable improvements to the movement of the linear stepper machine. Indeed, the rotor has reached its target position virtually without oscillations.

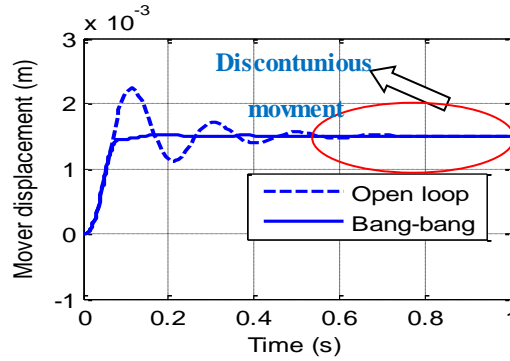


Fig.6- Waiting phase in open loop.

The control methods proposed in open loop, easy to implement, have greatly reduced oscillations and overruns and the mobile positioning accuracy. However, the mobile reaching its equilibrium position with a great delay, Figure.6, makes these control methods poorly suited for applications that require rapid positioning.

3. Improvement of the linear stepper motor positioning quality by the closed-loop control

The actuator-syringe assembly mechanical equation is of the form, [3-10-11-12]:

$$m_c \frac{dx^2}{dt^2} = F(i, x) - \xi \frac{dx}{dt} - F_0 \text{signe} \left(\frac{dx}{dt} \right) - F_c \quad (1)$$

With $F_c = m_s \frac{dx^2}{dt^2} + C_1 x \frac{dx}{dt} + C_2 \left(\frac{dx}{dt} \right)^2 + C_3 \frac{dx}{dt}$ is the load force developed by the syringe, [13-14-15-16].

To synthesize the transfer function, it is considered that the machine operates at a vacuum $F_c = 0$ and the mobile movement is ahead where $\text{sign}(V) > 0$ and $F_0 = 0$. Equation (1) becomes:

$$m_c \frac{dx^2}{dt^2} = F(i, x) - \xi \frac{dx}{dt} \quad (2)$$


The transfer function between the position x and the thrust force F is given by, [4].

$$m_c s^2 x(s) + \xi s x(s) = F(s) \quad (3)$$


$$G(s) = \frac{x(s)}{F(s)} = \frac{1}{m_c s^2 + \xi s} \quad (4)$$

Moreover, the thrust force developed by one phase is expressed by:


Simulation results for a time of the order of unity infusion, Figure.8 illustrates the dynamic behavior of the assembly from control current, position, speed and thrust force on a whole step.

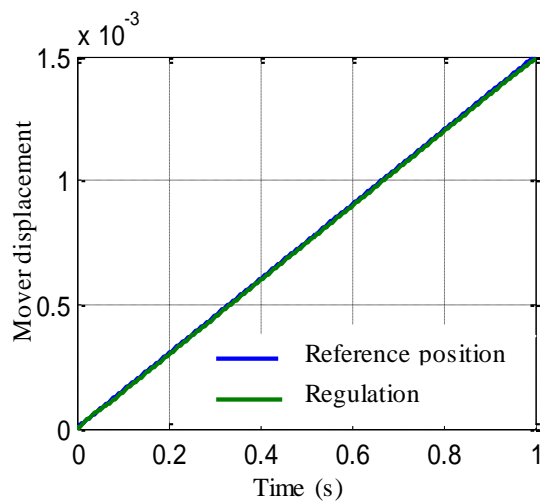

(a)

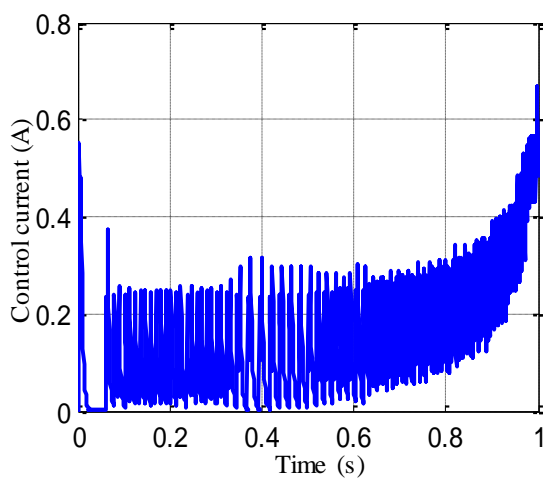

(b)

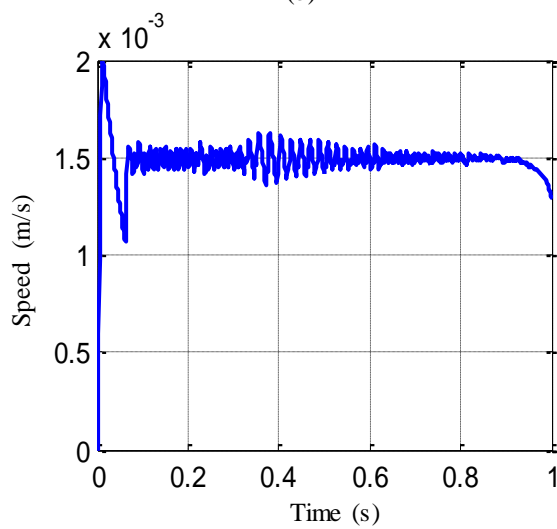

(c)

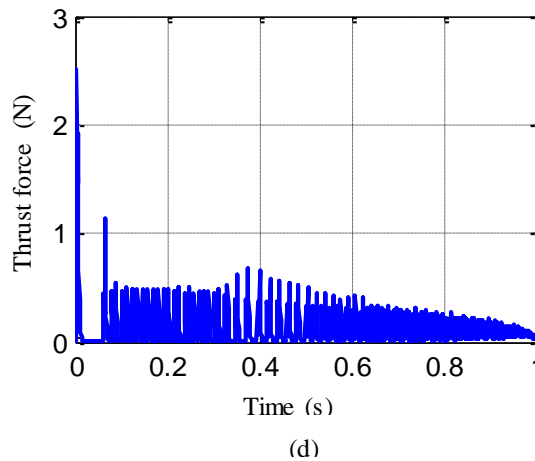


Fig.8– Closed loop control: Dynamic performance of the actuator for 1s infusion time

(a) : Mover displacement (b) : Control current (c) : Speed (d) : Thrust force.

In the case of a linear reference, the rotor movement is also perfectly linear. It can be observed that the control law functions correctly with a trajectory tracking with a very good precision, figure 8 (a). As expected the current is chopped to satisfy the motion linearity, Figure.8 (b). The average speed remains constant around $1.510^{-3}m/s$, figure.8 (c). As for the Thrust force, it remains positive average value canceling at the end of the step which is consistent with the principle of operation, Figure.8 (d). On the other hand, the excitation of the phase A allows the positioning of the actuator on the first equilibrium position corresponding to 1.5 millimeters. The successive excitation of the other phases is necessary for the next positions.

The closed-loop control has therefore brought undeniable improvements to the linear stepper movement and the control strategy has led to satisfactory results.

The dynamic performances of the all biomedical system during an infusion depend on the interaction of several parameters characterizing the volume of infusion $V_{infusion}$, the syringe geometry ($L_c = 118mm$ and $V_c = 60ml$) and the Tooth pitch of the actuator $\lambda = 6mm$. These parameters are related by the following expression:

$$V_{infusion} = \frac{\lambda}{L_c} V_c \quad (9)$$

Table 3. Infusion Volume versus infusion time and the number of cycles.

Number of power cycles	Infusion Volume (ml)	Infusion time (s)
1	1.5	4
2	3	8
3	4.5	12
4	6	16
...
20	30	80

Table 3 shows that the infusion time is proportional to the volume of aqueous solution to be infused. For instance, an infusion volume of 1.5 ml of sodium chloride corresponds to an infusion time of four seconds which requires one power cycle of the actuator. According to the nature of the disease and the patient, the infusion volume is increased or decreased and consequently the infusion time. In this case, it is necessary to repeat or split the power cycle of the actuator according to the need.

4. Conclusion

The development of control methods for improved motion performance of LSRM is the purpose of this article. The first part is devoted to the study of conventional technique commonly used for the damping of rotor oscillations. However, this approach does not solve the problem of the movement regularity, an essential factor characterizing the medical application. To overcome the limitations and inadequacies of conventional control techniques, a control concept based on closed-loop control is developed in the second part. The application of this control strategy made it possible to enslave the system and force it to follow rigorously the linear reference without overshoots and without oscillations.

References

1. P. SCHERPEREEL. "Le diabète est-il un facteur de risque à l'opération", Congrès National d'Anesthésie Réanimation, pp.31-40, Ed. Masson. Paris, 1991.
2. B. BEN SALAH, M. N. ABDELKRIM. "Sur la régulation de la perfusion des pousse-seringues pilotés par moteur pas à pas ", International Conférence on Electronic Engineering, Oran, 1994, pp.196-202
3. M. JUFER, "Electromécanique", Presses Polytechniques 1995, Universitaires Romandes, Lausanne.
4. P. ACARNLEY, "Stepping motors a guide to theory and practice", The Institution of Electrical Engineers, Edition IEE, London 2002.
5. Y. Peng, J. Cao¹, Z. Guo¹ and H. Yu, "A linear actuator for precision positioning of dual objects", Smart Materials and Structures 24 (2015) 125039 (9pp).
6. J. MARIDOR, " Design, Optimization, and Sensorless Control of a Linear Actuator", PHD thesis, école polytechnique fédérale de lausanne, 2011.
7. K.TAKASHI, " Stepping motors and their microprocessor controls", Clarendon press, Oxford 1984, ISBN 0-19-859326-0.
8. S. Imen, H. Mohamed Ali and S. Dhaou, " Design and control of a linear switched reluctance actuator of motorization a left ventricular assist device.", Biomedical Research 2018; 29 (11): 2327-2336.
9. B. Ben Salah., K. Ben saad, M. Benrejeb, " Sur une approche de lissage du mouvement incrémental des moteurs pas à pas linéaires", 2^{ème} Journées Scientifiques des Jeunes Chercheurs en Génie Electrique et Informatique, GEI' 2002, Hammamet.
10. Z. Wajdi, " Commande d'un moteur linéaire pas à pas à réluctance variable en vue d'une implémentation ", Mastère Electrotechnique et Systèmes Industriels, ESSTT, septembre 2011.
11. T. R. Fredriksen, "Application of the Closed-Loop Stepping Motor", IEEE Trans. on Automatic Control, vol. AC-13, pp. 464-474, Oct. 1968.

12. Z. Wajdi, K. Jalel and R. Habib, "Speed control of linear switched reluctance motor", World Congress on Computer and Information Technology (WCCIT), 2013.
13. J .P. FAROUX, J. RENAULT, "Mécaniques des fluides et ondes mécaniques ", Dunod, Paris, 1999, ISBN 2-10-003434-0, 2ème années PC.
14. [M. Imed, R. Habib and M. AYADI, "Design and modelling of a linear switched reluctance actuator for biomedical applications" International Journal of the Physical Sciences Vol. 6(22), pp. 5171-5180, 2 October, 2011.
15. J. FAISANDIER, "Mécanismes hydrauliques et pneumatiques", Dunod, Paris, 1999, ISBN 2-10-004074-X 8^{ème} édition.
16. M. Imed, "Design and modelling of a LSRM for biomedical applications": ISBN 978-3-659-15449-2, LAP LAMBERT Academic Publishing GmbH & Co. KG Heinrich-Böcking-Str. 6-8 66121 Saarbrücken Germany. Fon +49 681 3720-310, Fax +49 681 3720-3109. www.lap-publishing.com, June 2012.
17. , Z. Wajdi, M. Imed, F. Mourad and R. Habib, " Control of linear switched reluctance motor for biomedical application, International Conference on Electrical Engineering and Software Applications (ICEESA 2013), 21-23 March 2013, Hammamet, Tunisia.
18. P. Luís Miguel, C. Maria do Rosário and M. Sílvio "Speed Control Scheme Analysis of Switched Reluctance Actuator", PRZEGLĄD ELEKTROTECHNICZNY (Electrical Review), ISSN 0033-2097, R. 88 NR 1a/2012.
19. Dr. RAMA RAO, Ms. D. SAILAJA, Mr. P. DEVIKIRAN Et Mr. A. PHANI KUMAR, "Closed Loop Speed Control of 6/4 Pole Switched Reluctance Motor", International Journal of Emerging Trends in Electrical and Electronics (IJETEE – ISSN: 2320-9569) Vol. 10, Issue. 10, Oct. 2014.
20. P. Bala Koteswararao et J. Hema Sunder, " A Closed Loop Speed Control of a Switched Reluctance Motor with a New Converter Topology", International Journal of Emerging Technology and Advanced Engineering, Volume 3, Issue 9, September 2013.
21. J.F. Pan , Norbert C. Cheung et Yu Zou, "High-precision control of LSRM based X–Y table for industrial applications", ISA Transactions 52 (2013) 105–114.
22. P. Prasanna Lakshmi et L. Ravisrinivas, "Modeling and Simulation of Switched Reluctance Motor Double Closed Loop Control System", International Journal Of Innovative Research & Development, Vol 1 Issue 8, October, 2012.

Authors' information

Imed MAHMOUD was born in Mahdia, Tunisia, on 04 Mars 1982. He received the Diploma of Baccalaureate in applied science degree in 2002 at Secondary School Souassi Mahdia, the M.Sc. degree in 2006, in Electrical Engineering option Electrical engineering and Power Electronics and Master degree in Electrical engineering and Systems Industrial 2008 and the doctoral degree in 2015, all from the ESSTT (High School of Sciences and Technology of Tunis), University of Tunis, Tunisia. He joined the teaching staff of the ESSTT in 2008. His main research interests are study, design, modelling and control of linear actuators.



Adel Khedher was born in Mahdia, Tunisia in 1967. He received Master of Sciences Degree and DEA from ENSET, Tunis, Tunisia, in 1991 and 1994, respectively, Ph.D. and HDR from ENIS, Sfax, Tunisia in 2006 and 2012 respectively. From 1995 to 2002, he had been a training teacher in the professional training centers. From 2003 to 2006, he had been an Assistant professor in the Electronic Engineering Department of ISSATS, Sousse, Tunisia. He has been promoted to the associate professor grade in the same department since June 2006. From September 2010, he has been an associate professor in the Industrial Electronic Engineering Department of ENISO, Sousse, Tunisia. He has been promoted to the Full professor grade in Electrical Systems in the same department since November 2012. His main research interests cover several aspects related to control of the Static Converters, the Electric Machines Drives and the Renewable and Green Energies Systems. I published in this field more than twenty indexed papers. I have been teaching renewable energy subjects to engineering students, master and doctoral ones for more than five years. The program focuses on wind, photovoltaic and green energies.